

Particle Counter With Camera User Manual



**Please read this manual before switching the unit on.
Important safety information inside.**

Contents

1.Introduction.....	4
2.Features.....	4
3.Specification.....	5
4.Front Panel And Button Description.....	6
5.Power on or Power off.....	6
6.Measurement Mode.....	6
7.Particle Counter measurement mode.....	8
8.Storage File Browser.....	11
9.System Settings.....	12
10.Help File.....	15

1.Introduction

Thank you for purchasing this Particle Counter instrument. This instrument is Particle Counter with 2.8" color TFT LCD display & a microSD memory card for capturing images (JPEG) or video (3GP) for viewing on your PC. Providing fast, easy and accurate readings for particle counter, air temperature & relative humidity, most surface temperature measurements. It is the first combination of these measurements in global. Would be the best instrument for environment protection and energy save. The dewpoint temperature measurement will be very visible for wet and dry proof. It is a good hand industrial measurements and data analyzing, the real scene and time can be displayed on color TFT LCD. Any memory readings can be recorded in SD card. The user can be back in office to analyze the measured air quality under the support of software.

2.Features

- 2.8" TFT Color LCD display
- 320*240 pixels
- Images (JPEG) & Video (3GP)
- MicroSD (max, use 8GB) memory card
- Simultaneously measure and display 6 channel of particle sizes.
- Air temperature and humidity
- Dewpoint & Wetbulb temperature
- MAX, MIN, DIF, AVG record, Date/time setup controls
- Auto Power Off

3. Specifications

Particle Counter	
Channels	0.3,0.5,1.0,2.5,5.0,10um
Flow Rate	0.1ft ³ (2.83L/min)
Counting Efficiency	50% @ 0.3 μ m; 100 % for particles > 0.45 μ m
Coincidence Loss	5% at 2,000,000 particles per ft ³
Data Storage	5000 sample records (MicroSD card)
Count Modes	Cumulative, Differential,Concentration,

Air temperature and Relative humidity measurement	
Air Temperature Range	0°C to 50°C(32°F to 122°F)
Dewpoint Temperature Range	0°C to 50°C(32°F to 122°F)
Relative Humidity Range	0 to 100%RH
Air temperature Accuracy	±0.5°C(0.9°F) 10°C to 40°C
	±1.0°C(1.8°F) others
Dewpoint temp. Accuracy	±0.5°C(0.9°F) 10°C to 40°C
	±1.0°C(1.8°F) others
Relative Hum. Accuracy	±3%RH 40% to 60%
	±3.5%RH 20% to 40% and 60% to 80%
	±5%RH 0% to 20% and 80% to 100%
Operating Temperature	0°C to 50°C(32°F to122°F)
Storage Temperature	-10°C to 60°C(14°F to 140°F)
Relative Humidity	10 to 90%RH non-condensing
Display	2.8"320*240 Color LCD with backlight
Power	
Battery	Rechargeable battery
Battery Life	About 4 hours continuous use
Battery Charge Time	About 2 hours with AC adapter

4. Front Panel And Button Description




5. Power on or Power off

On the power off mode, press and hold  button, until the LCD is on, then the unit will power on.
On the power on mode, press and hold  button, until the LCD is off, then the unit will power off.

6. Measurement Mode

This instrument has three modes

On the power on mode, the unit will display the three measure modes, and display three setup options. You can use  or  button to select any measure mode you need, and use function button F1, F2, F3 to enter the system interface.

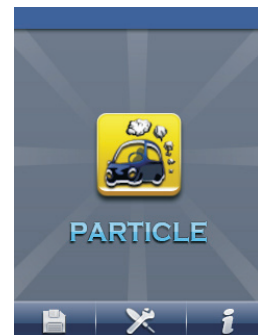

Items	Description
	Memory Set
	System Set
	Help file


Symbols

Symbol	Description	Symbol	Description
	Cumulative mode		Differential mode
	Concentration mode		Scan
	HOLD		Alarm working
	CAM mode		Video mode

7. ParticleCounter measurement mode

On the power on mode, you can press the ENTER button to enter the Particle Counter mode, Start to measure and display temperature and humidity.

Press RUN/STOP button to start detection of particles, when the sample time is up, the particle measurement will automatically stop, and the data will automatically save. You can also press RUN/STOP button to stop the measurement when the sample time is not up. This mode can take picture and take video

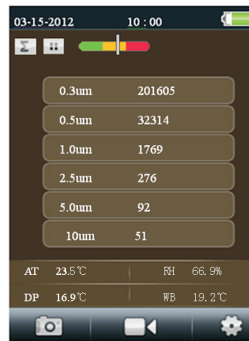

7.1 Take picture function


On the particle counter mode, you can see  icon, and these icon corresponding to F1, F2, F3 button, press F1 button can enter picture taking,  icon will appear, you can press F2 button to take picture. Press "ESC" button to exit this mode.

7.2 Take video function

On the particle counter mode, you can see  icon, and these icon corresponding to F1, F2, F3 button. press F2 button can enter video taking mode, Press the RUN/STOP button to start the particle measurement, the instrument start to measure the particle, The LCD display  icon, press F2 button to take video and press F2 button again to stop take video, The video file will be auto to saved. Press ESC button to exit this mode.


7.3 Particle Setup mode

On the particle counter mode, you can see  icon, and these icon corresponding to F1, F2, F3, press F3 can enter the setup mode, on this mode, you can setup any parameter you want. Use the ▲ or ▼ button to select any option you want to setup. Then press ENTER button to confirm the parameter.

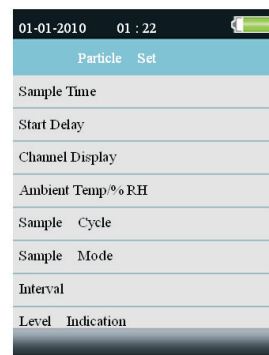


Sample time

You can adjust the sample time use the ▲ or ▼ button to control the volume of measured gas. It can be set to 60s/2.83L.

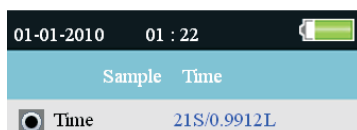


Start Delay

You can adjust the time use the ▲ or ▼ button to control start time. The delay time of up to 100 seconds.

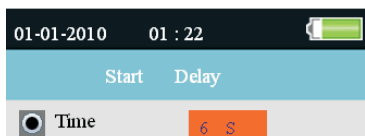


Channel Display

This setting to select the channel is being displayed. Use the or button to select channel and use ENTER button to confirm.

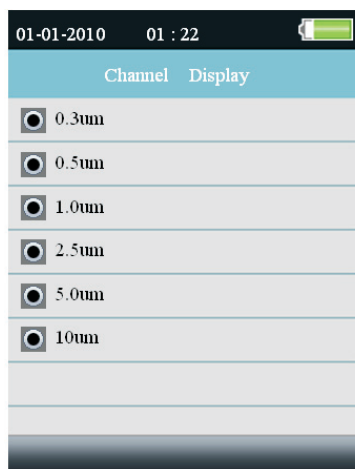


Ambient Temp/%RH

Choose this setting if the Air temperature and humidity are displayed..

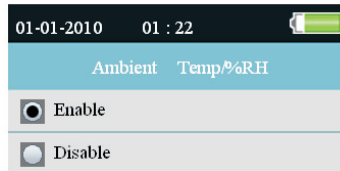


Sample Cycle: This option is used to set the sampling period.

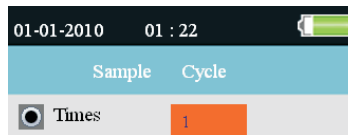


Sample Mode

This setting is used to set the display mode of particle counter. When you select the cumulative mode, the particle measure will display  symbol and the meter work in the cumulative mode. When you select the differential mode, the particle measure will display  symbol and the meter work in the differential mode. When you select the concentration mode, the particle measure will display  symbol and the meter work in the concentration mode.

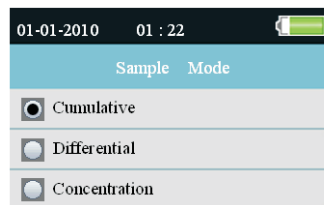


Interval

Set the time between samples for the sampling period is greater than one times. The longest interval is 100 seconds.

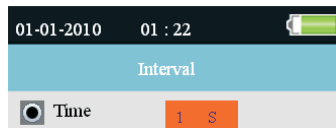

Level Indication

Select the alarm level of the corresponding particle size in the measurement, when the selected particle size exceeded, the instrument measuring interface will have exceeded the prompt.

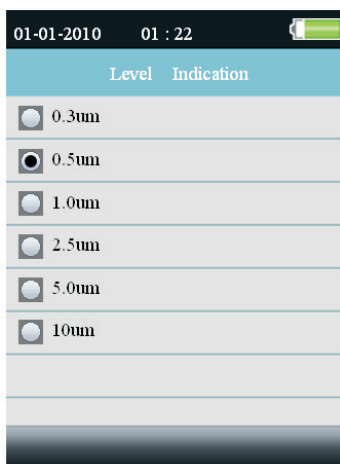


8.Storage File Browser

Turn the instrument on, below the LCD has a bar icon.    Click on the  icon to enter the data memory via the F1 button. On the Memory set mode, there are three options, press ▲ or ▼ button to select one and press ENTER button to enter this option. And then you can view the recorded data, images, and video information. If you do not save the information, it shows no file.

9.System Settings

Turn the instrument on,below the LCD has a bar icon.
icon to enter the System Set Mode via the F2 button.

   Click on the 

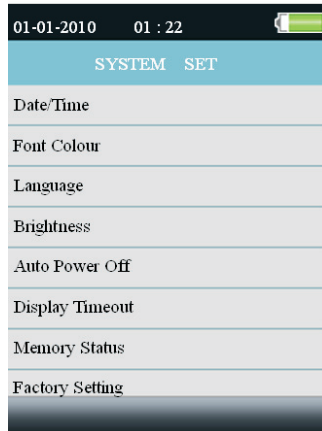


Items	Descriptions
Date/Time	Set date and time
Font Colour	Select the font colour
Language	Select Language
Brightness	Brightness adjustment
Auto Power Off	Select auto power off time
Display Timeout	Select display auto off time
Memory Status	Display the memory and MicroSD card capacity
Factory Setting	Restore factory settings
Units(°C/°F)	Select the temperature unit

Press the ▲ or ▼ button to select the items,Then press the ENTER button to enter

9.1 Date/Time

Press the ▲ or ▼ button to select the value,press ENTER button to set the next value,press ESC button to exit and save the date and time.

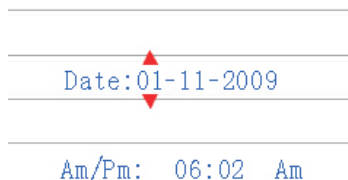

9.2 Font Colour

Press the ▲ and ▼ button to select the color, press the ESC button to esc and save.




9.3 Language

Press the ▲ and ▼ button to select language, press the ESC button to esc and save.


9.4 Brightness

Press the ▲ and ▼ button to select the backlight brightness, press the ESC button to esc and save.

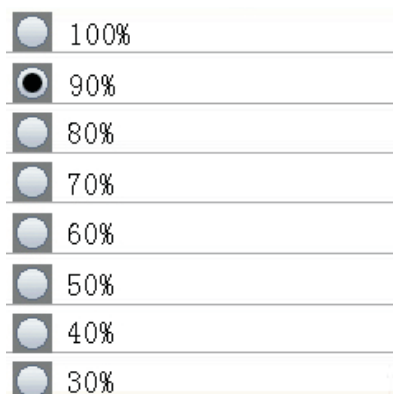

9.5 Auto Power off

Press the ▲ and ▼ button to select the auto power off time or never auto power off, press the ESC button to esc and save.

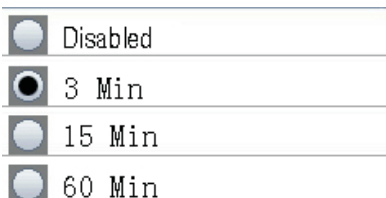

9.6 Display Timeout

Press the ▲ and ▼ button to select the Display auto off time or never Display auto off, press the ESC button to esc and save.

☒	Disable
☐	90s
☐	2 Min
☐	4 Min

9.7 Memory Status

Press the ▲ and ▼ button to select the memory (flash or microSD). Press the ESC button to esc and save.

☒	Device
☐	SD Card
Total:	[74] MB
Used:	[0] MB
Free:	[74] MB (100%)

NOTE: If MicroSD card inserted, MicroSD card will be selected by default

Press the ENTER button to format the flash or MicroSD card, press **F3** button to cancel format, press **F1** button to confirm format.

9.8 Factory Setting

Press the ▲ and ▼ button to select yes or no restore factory settings. Press the ESC button to esc and save.

☐	No
☒	Yes

9.9 Units(°C/°F)

Press the ▲ and ▼ button to select the unit, press the ESC button to esc and save.



10.Help File

This is Particle Counter with 2.8" color TFT LCD display & a microSD memory card for capturing images(JPEG) or video(3GP)for viewing on your PC. Providing fast,easy and accurate readings for particle counter,air temperature & relative humidity,most surface temperature measurements. It is the first combination of these measurements in global,would be the best instrument for environment protection and energy save.The dewpoint temperature measurement will be very visible for wet and dry proof.It is a good hand industrial measurements and data analyzing, Any memory readings can be recorded in SD card.The user can be back in office to analyze the measured air quality under the support of software.

10.1 Particle Counter instruction



1.Particles that scattered in the dust in the air,dust or smoke.They mainly come from automobile exhaust,power plant,garbage incineration furnace and so on.Relative diameter less than 2.5um particles known as PM2.5,this particle is smaller than human cells,not be drained,but directly into the lungs and blood,the harm to human body is larger.

2.This meter with a simple key operation to achieve a particle counter measurement, real-time monitoring the value of environmental particles concentration, six channel data measured simultaneously,and at the same time displayed on the screen, also can be a separate display.Joined the exceed the standard grade alarm indication,and accompanied by different buzzer,more direct master of environmental quality.

3.Equipped with cameras and photographic function,can directly see measured the real situation, can store large amounts of data (SD), pictures and video, is used to analyze the data

4. Due to particulate matter measurements need to start the pump, will be dust inhalation, is recommended for daily use less as far as possible, to reduce the pollution on the sensor, thereby increasing the service life of the instrument, such as the average daily use 5 times, the instrument can be used for 5 years.

Attention: in the foggy there will be fine mist as dust!

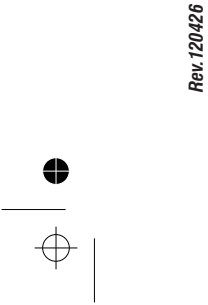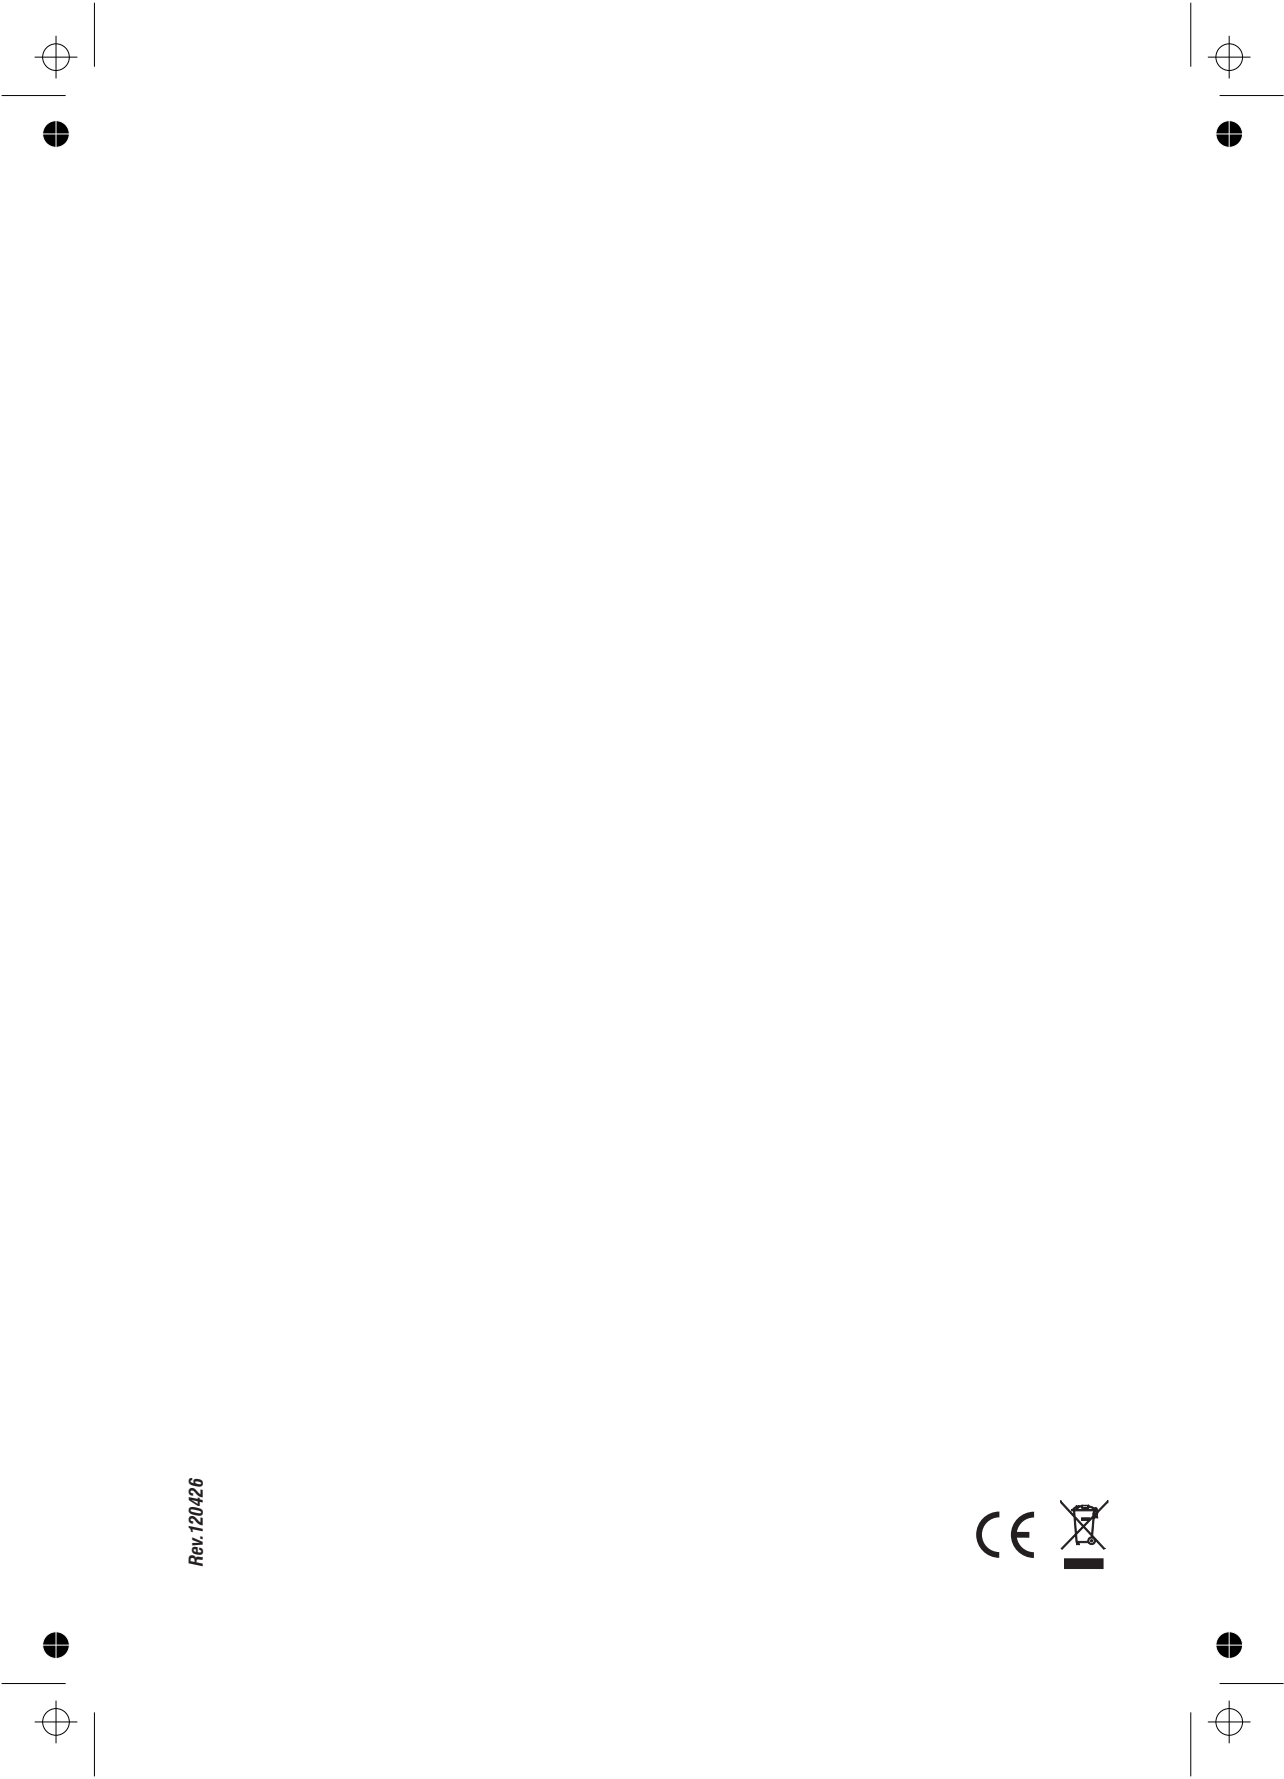

Rev.120426

